

1/4

Fig. 1

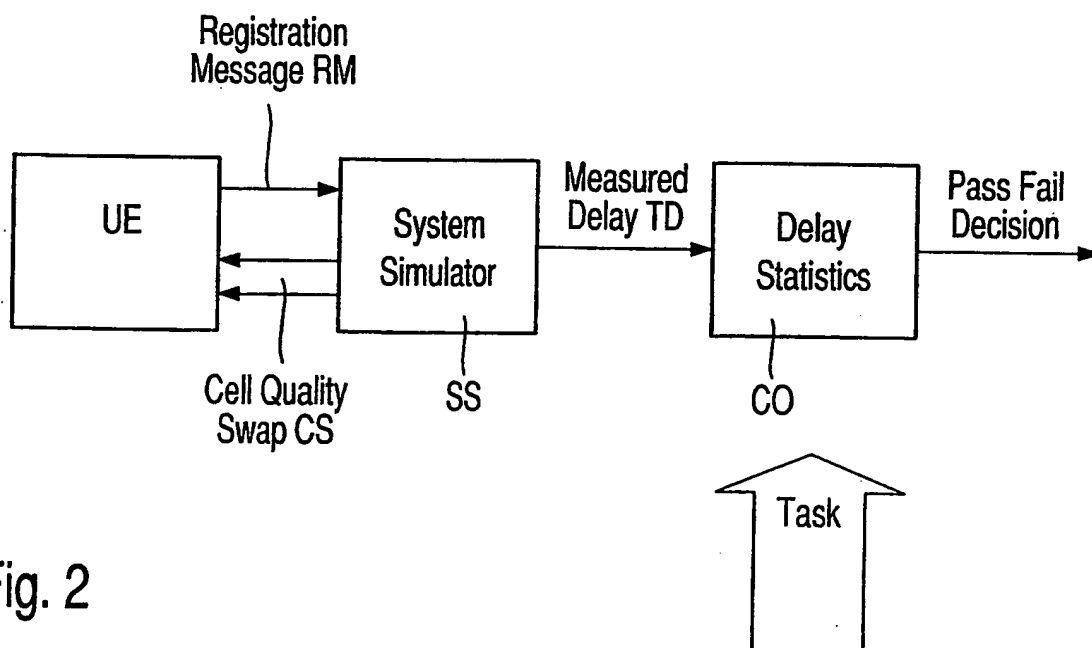
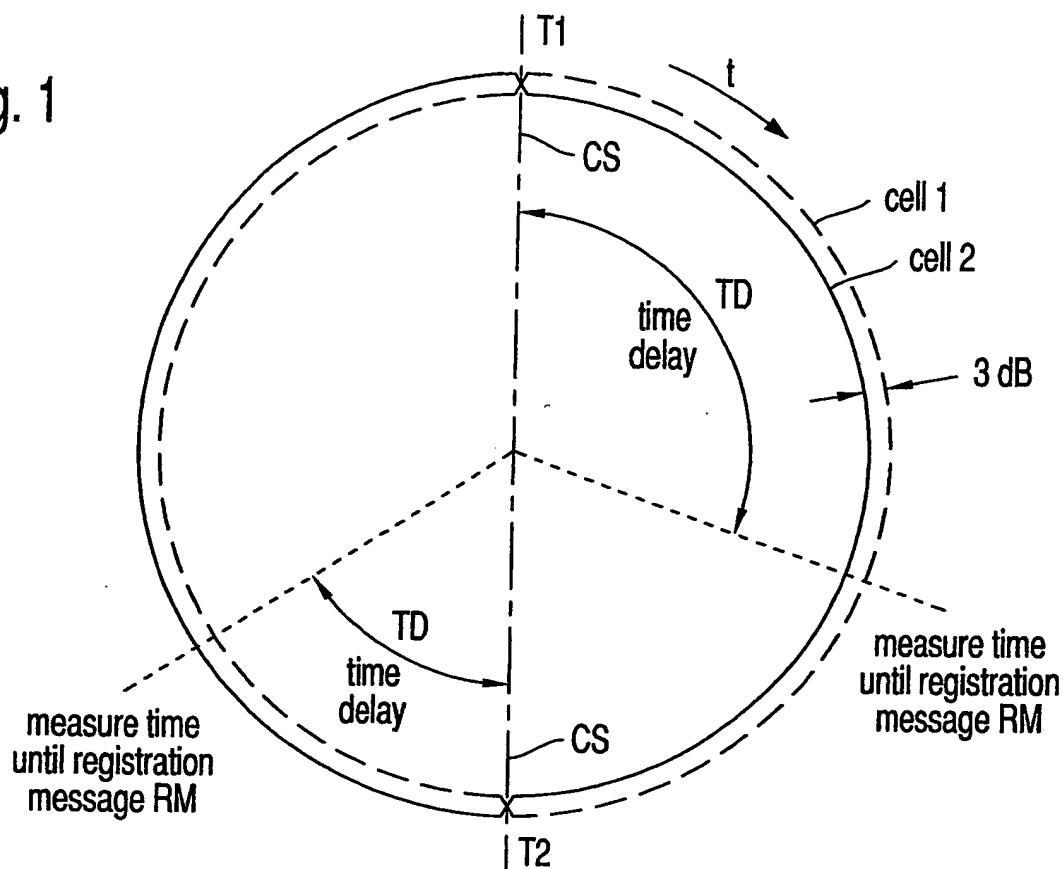


Fig. 2

2/4

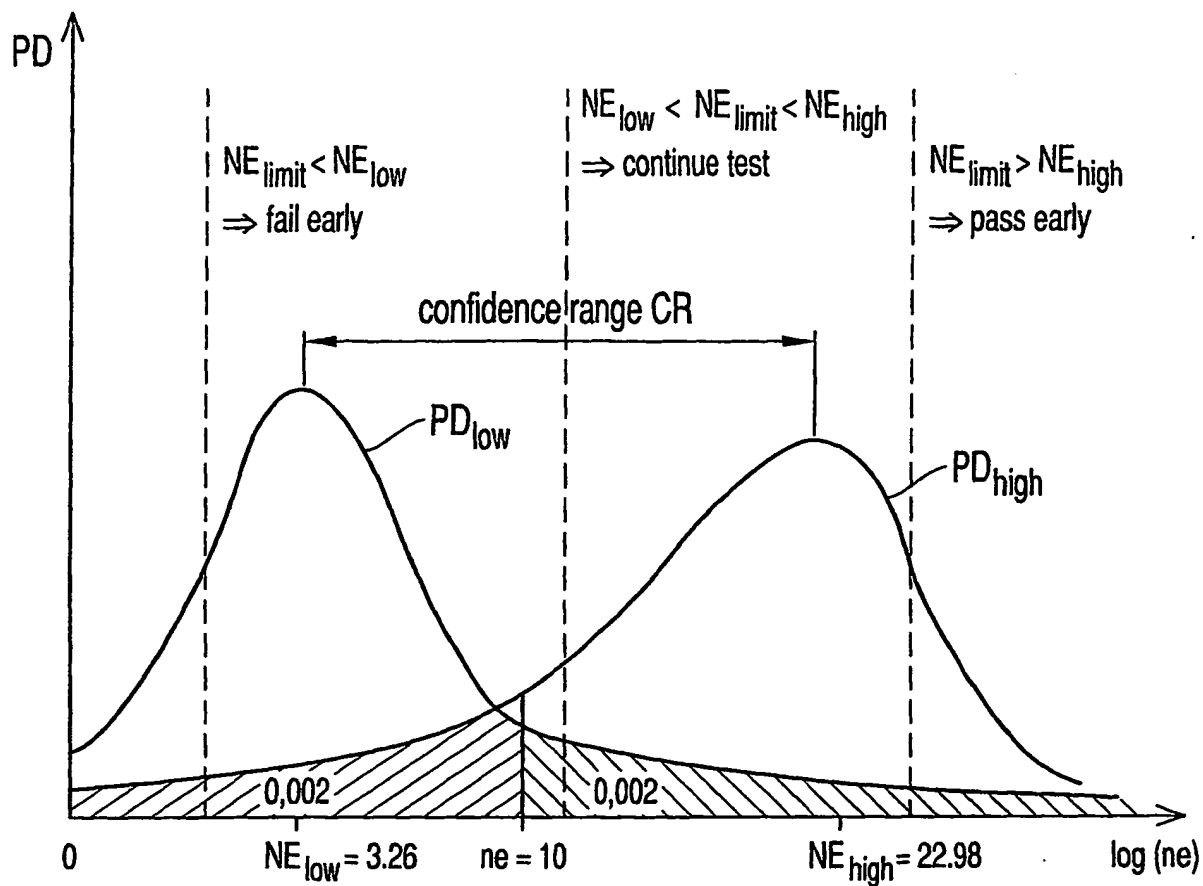


Fig. 3

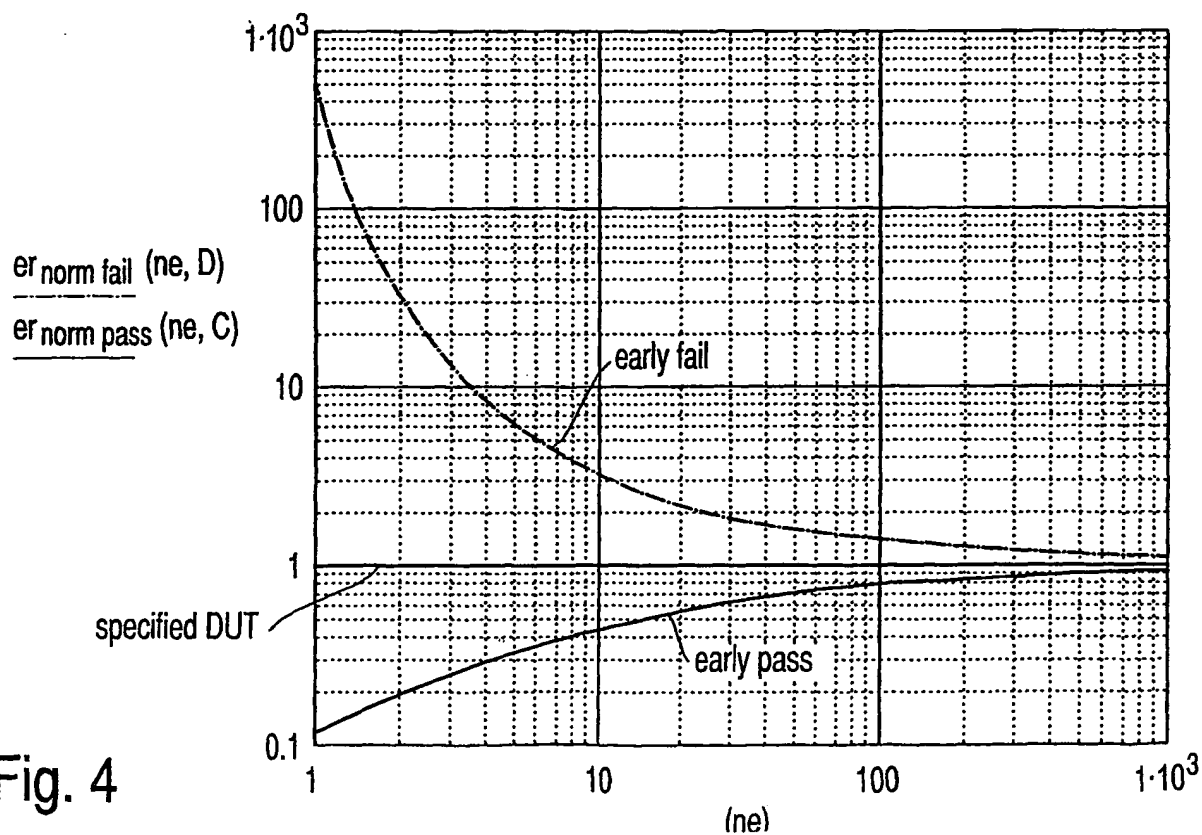


Fig. 4

3/4

ER limit = 0.2 (1/5) Actual ER = 0.25 (1/4)

Number of sample,	1	2	3	4	5	6	7	8	9	10 etc...
Sequence, 0: correct, 1: error	0	1	0	0	0	1	0	0	0	1
ER		1/2	1/3	1/4	1/5	2/6	2/7	2/8	2/9	3/10
ER <sub>norm</sub>		5/2	5/3	5/4	5/5	10/6	10/7	10/8	10/9	15/10

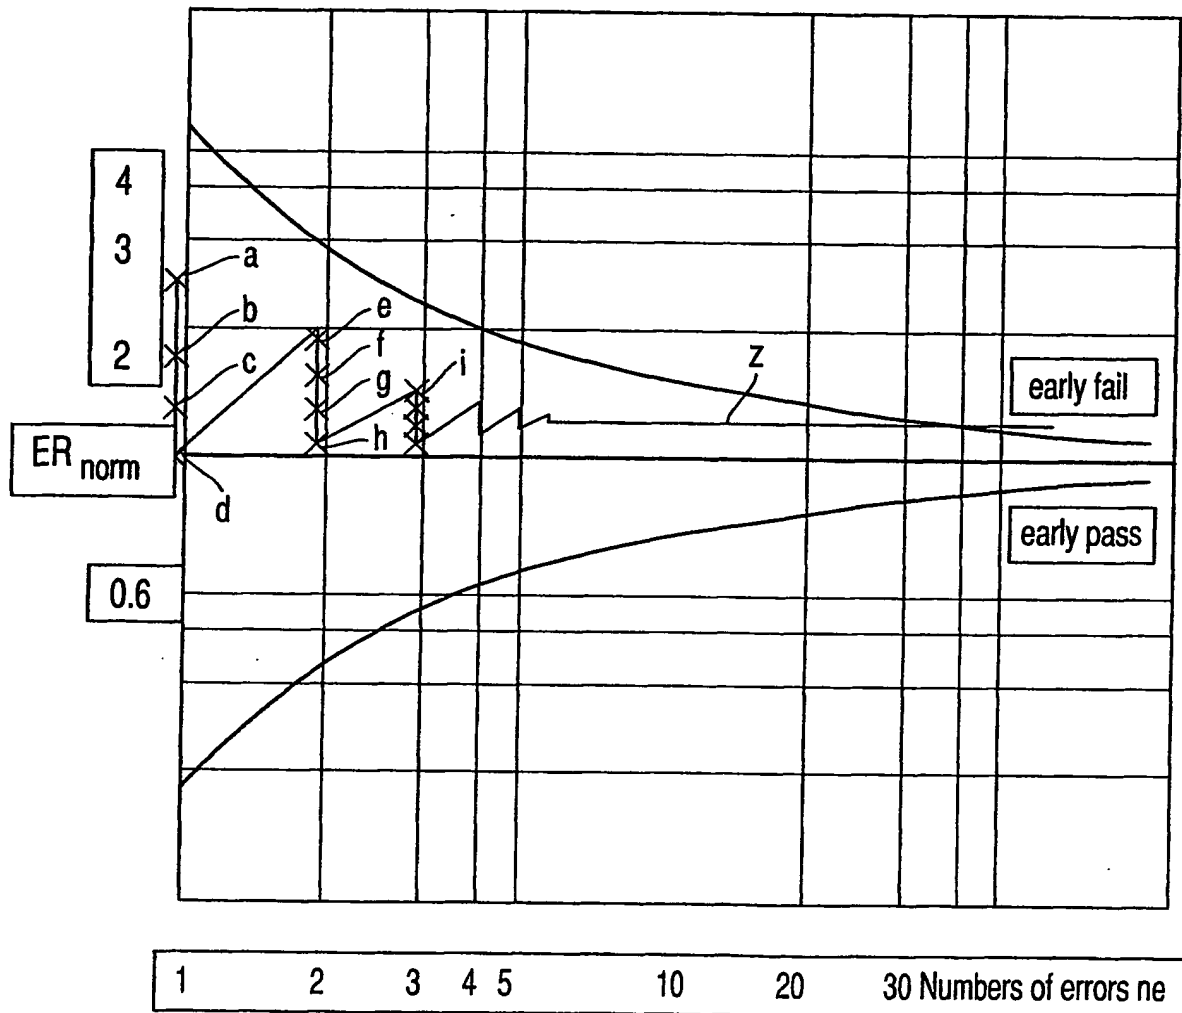


Fig. 5

4/4

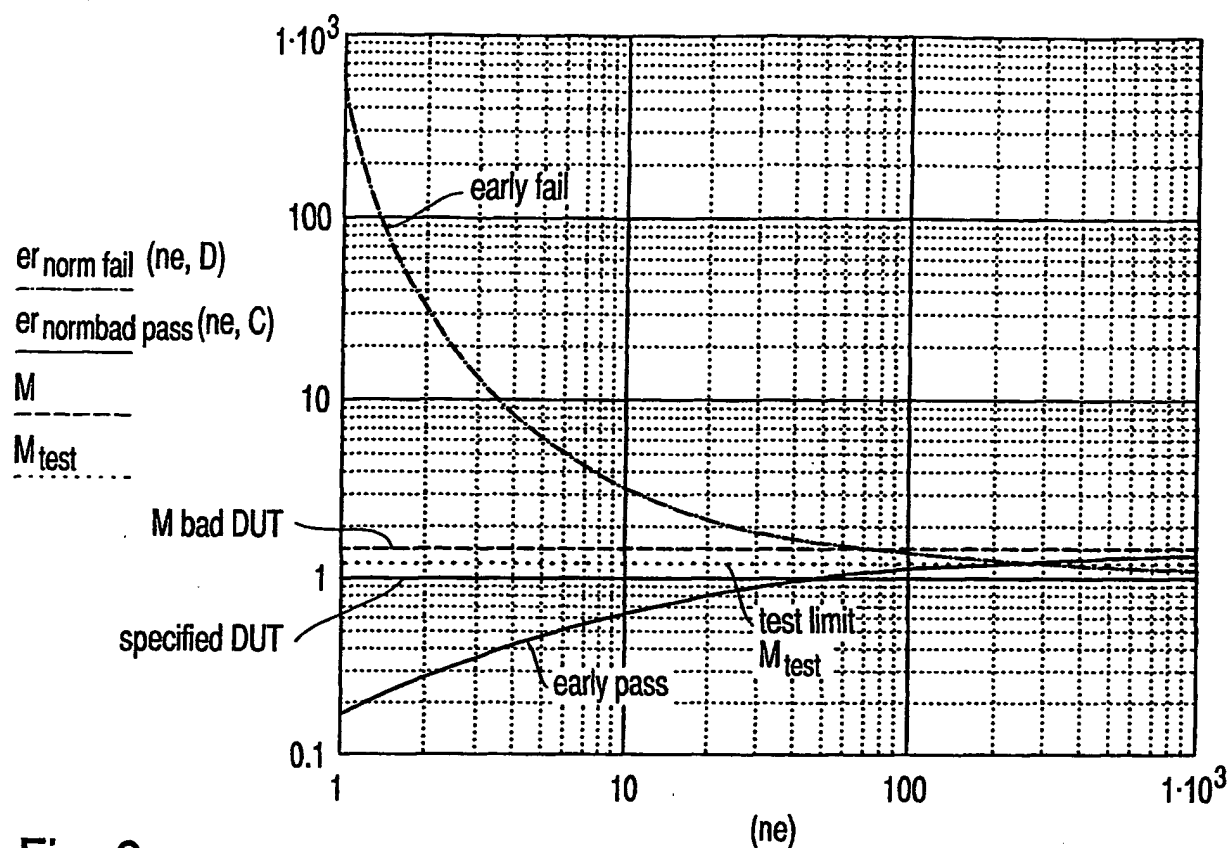


Fig. 6

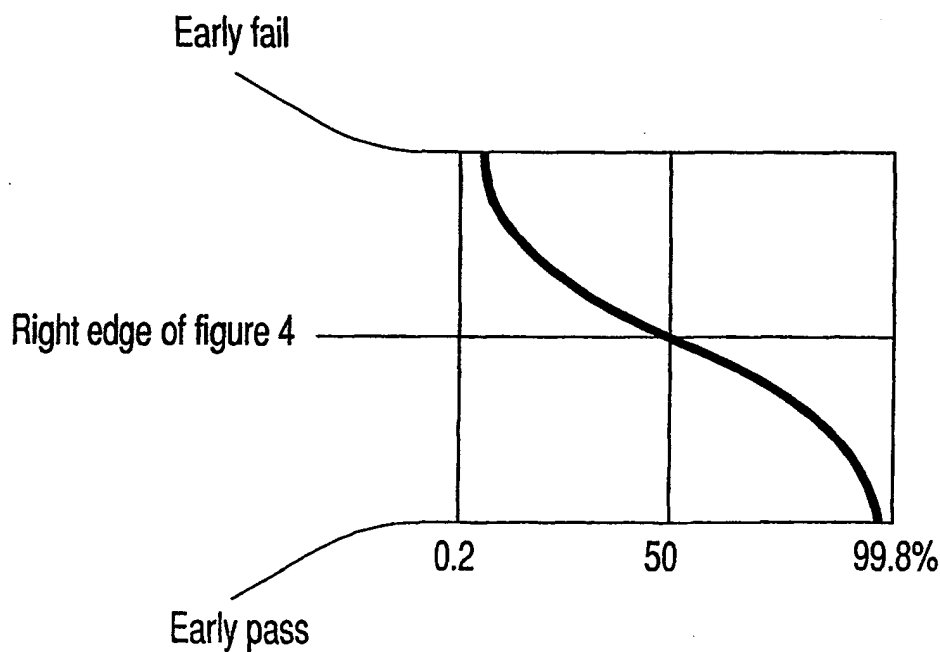


Fig. 7